

APPLICATION NOTE

Test for Line Width and Gyromagnetic Ratio

Introduction

At a constant microwave frequency ($\omega = 2\pi f$), ferrimagnets exhibit electromagnetic energy absorption that is a function of the internal static magnetic field (H_i). Maximum absorption occurs when the precession frequency and direction of the elementary magnetic dipoles equals that of the incident microwave magnetic field. The magnitude of H_i (H_r) required to obtain maximum absorption (i.e., the ferromagnetic resonance condition) can be computed from the following equation:

$$\omega = \gamma_{\text{eff}} H_r \quad (1)$$

Where:

- $\omega = 2\pi \times$ the resonant frequency
- γ_{eff} = Effective gyromagnetic ratio
- H_r = Magnitude of H_i

For a spherical test specimen, H_i is independent of the material magnetization and may be taken as equal to the applied Direct Current (DC) magnetic field.

The ferrimagnetic resonance line width (ΔH) is defined as the separation of the two H_i values at which the power absorbed by the ferrimagnet is equal to half the maximum absorption, as shown in Figure 1.

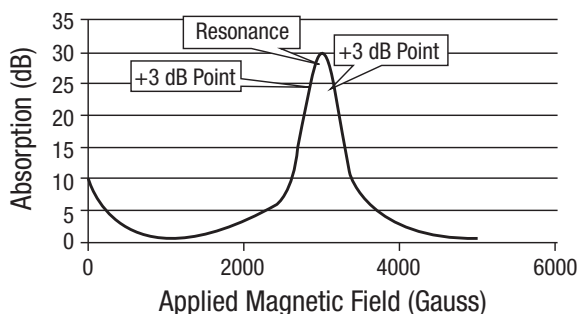


Figure 1. Ferrimagnetic Resonance for a Sphere at 9300 MHz

Cavity Method

The A TE_{10n} (n even) cavity resonant in the X-band region is used, or alternatively is the H-field maximum in the coupling iris of a cross-guide coupler. The Loaded Q (QL) of the empty cavity should be 2000 or greater. The test sample is a sphere that is a diameter of approximately 0.040 inches. The cavity technique requires that the sample be small compared to one-quarter of the wave-length (λ) of the microwave radiation within it:

$$\lambda = 3 \times 10^4 / f(\epsilon')^{1/2} \text{ [cm]} \quad (1)$$

Where:

- λ = Wavelength (cm)
- f = Frequency in megacycles
- ϵ' = Dielectric constant
- cm = Centimeters (dimension which the wavelength is measured)

The sample, mounted on a fused silica or equivalent rod, is positioned away from the cavity wall at a point of minimum microwave electric and maximum microwave magnetic field. A power meter can be used to read off the half-power points by adjusting the DC magnetic field and measuring the difference in field directly.

Measurement

Measurement is carried out at a fixed frequency, and the DC field from an electromagnet of suitable homogeneity is adjusted until the specimen is at ferromagnetic resonance (peak absorption). Using Equation (1) the gyromagnetic ratio can be initially determined from the measurement frequency and the resonance field. This characteristic may also be given in terms of $\gamma_{\text{eff}} = \gamma_{\text{eff}} \times 2mc/e$, (MKS units).

The width of the ferromagnetic resonance is found by sweeping the magnetic field through resonance, and measuring the DC field at the half-power (+3 dB) point using an accurate Gaussmeter. Trans-Tech, Inc. (TTI) uses a Noise Margin Reading (NMR) based instrument. The exact peak is then found by differentiating the DC field/power plot digitally and the +3 dB points determined precisely using a polynomial curve fitting, which eliminates operator error in setting and reading the peak and +3 dB points.

APPLICATION NOTE • TEST FOR LINE WIDTH AND GYROMAGNETIC RATIO

Because the +3 dB line width is sensitive to temperature, the measurement must be carried out in a temperature-controlled room, and the magnet pole pieces are water-cooled to prevent heating. A thermocouple is used to measure the temperature at the specimen, which should ideally be controlled to within 1 °C to obtain an accuracy of 0.2 Oersted.

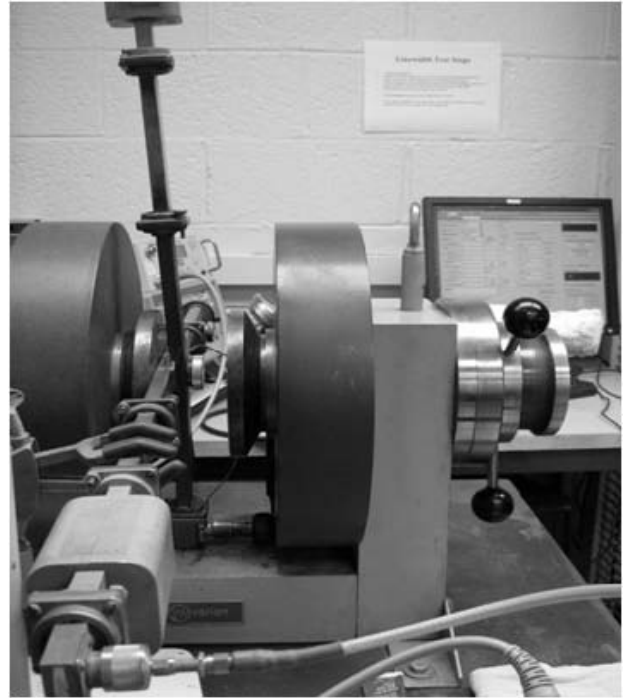


Figure 2. Typical Equipment Setup

Copyright © 2013, 2017 Trans-Tech Inc., All Rights Reserved.

Information in this document is provided in connection with Trans-Tech, Inc. ("Trans-Tech"), a wholly-owned subsidiary of Skyworks Solutions, Inc. These materials, including the information contained herein, are provided by Trans-Tech as a service to its customers and may be used for informational purposes only by the customer. Trans-Tech assumes no responsibility for errors or omissions in these materials or the information contained herein. Trans-Tech may change its documentation, products, services, specifications or product descriptions at any time, without notice. Trans-Tech makes no commitment to update the materials or information and shall have no responsibility whatsoever for conflicts, incompatibilities, or other difficulties arising from any future changes.

No license, whether express, implied, by estoppel or otherwise, is granted to any intellectual property rights by this document. Trans-Tech assumes no liability for any materials, products or information provided hereunder, including the sale, distribution, reproduction or use of Trans-Tech products, information or materials, except as may be provided in Trans-Tech Terms and Conditions of Sale.

THE MATERIALS, PRODUCTS, AND INFORMATION ARE PROVIDED "AS IS" WITHOUT WARRANTY OF ANY KIND, WHETHER EXPRESS, IMPLIED, STATUTORY, OR OTHERWISE, INCLUDING FITNESS FOR A PARTICULAR PURPOSE OR USE, MERCHANTABILITY, PERFORMANCE, QUALITY, OR NON-INFRINGEMENT OF ANY INTELLECTUAL PROPERTY RIGHT; ALL SUCH WARRANTIES ARE HEREBY EXPRESSLY DISCLAIMED. TRANS-TECH DOES NOT WARRANT THE ACCURACY OR COMPLETENESS OF THE INFORMATION, TEXT, GRAPHICS, OR OTHER ITEMS CONTAINED WITHIN THESE MATERIALS. TRANS-TECH SHALL NOT BE LIABLE FOR ANY DAMAGES, INCLUDING BUT NOT LIMITED TO ANY SPECIAL, INDIRECT, INCIDENTAL, STATUTORY, OR CONSEQUENTIAL DAMAGES, INCLUDING WITHOUT LIMITATION, LOST REVENUES OR LOST PROFITS THAT MAY RESULT FROM THE USE OF THE MATERIALS OR INFORMATION, WHETHER OR NOT THE RECIPIENT OF MATERIALS HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGE.

Trans-Tech products are not intended for use in medical, lifesaving, or life-sustaining applications, or other equipment in which the failure of the Trans-Tech products could lead to personal injury, death, or physical or environmental damage. Trans-Tech customers using or selling Trans-Tech products for use in such applications do so at their own risk and agree to fully indemnify Trans-Tech for any damages resulting from such improper use or sale.

Customers are responsible for their products and applications using Trans-Tech products, which may deviate from published specifications as a result of design defects, errors, or operation of products outside of published parameters or design specifications. Customers should include design and operating safeguards to minimize these and other risks. Trans-Tech assumes no liability for applications assistance, customer product design, or damage to any equipment resulting from the use of Trans-Tech products outside of stated published specifications or parameters.

Skyworks and the Skyworks symbol are trademarks or registered trademarks of Skyworks Solutions, Inc., in the United States and other countries. Third-party brands and names are for identification purposes only, and are the property of their respective owners.